

GORE® TAG®

Thoracic Branch Endoprosthesis

HOSPITAL INPATIENT CODING GUIDE 2024

Together, improving life



The reimbursement information provided by W. L. Gore & Associates, Inc. ("Gore") is presented for your convenience and general information purposes only. The information does not constitute legal advice and is subject to change without notice. The information is obtained from publicly available third-party sources and does not guarantee coverage or payment for services performed in any particular procedure utilizing any products manufactured or supplied by Gore.

Gore has used reasonable efforts to ensure the completeness and accuracy of the information contained herein as of the date this document was published. Health care providers are responsible for exercising their independent clinical judgment and following specific coverage guidelines and payer directives in selecting the codes that reflect the patient's condition and the services provided. Health care providers should contact the individual Medicare contractor or other third-party payer if they have questions regarding reimbursement. Gore does not promote its products outside of their FDA-cleared or approved labeled indications.

GORE® TAG® Thoracic Branch Endoprosthesis (TBE) description

TBE is indicated for endovascular repair of lesions of the descending thoracic aorta, while maintaining flow into the left subclavian artery.*

The GORE® TAG® Thoracic Branch Endoprosthesis is an implantable branched stent graft designed for branched thoracic endovascular aortic repair (TEVAR) of the descending thoracic aorta requiring placement into an area of the arch (zone 2) that includes the left subclavian artery. It consists of at least 2 components which line the thoracic aorta and the left subclavian artery. The devices allow blood to flow into the left subclavian artery and the rest of the aorta while preventing blood from flowing to the affected area and does not require an open surgical procedure. The device extends from the left subclavian artery, including a portion of the aortic arch, to the descending thoracic aorta.

The GORE® TAG® Thoracic Branch Endoprosthesis is made of expanded polytetrafluoroethylene (ePTFE) with an outer metallic support structure known as a stent. See *Figure 1* for an image depicting the GORE® TAG® Thoracic Branch Endoprosthesis.

FDA Breakthrough Device Designation

The device was granted priority review status on July 17, 2015. This was based on meeting required criteria:

- Intended to treat a potentially life-threatening disease
- Potential to provide a clinically meaningful advantage over existing legally marketed technology
- Offering significant clinically meaningful advantages over existing legally marketed alternatives
- Availability is in the best interest of patients

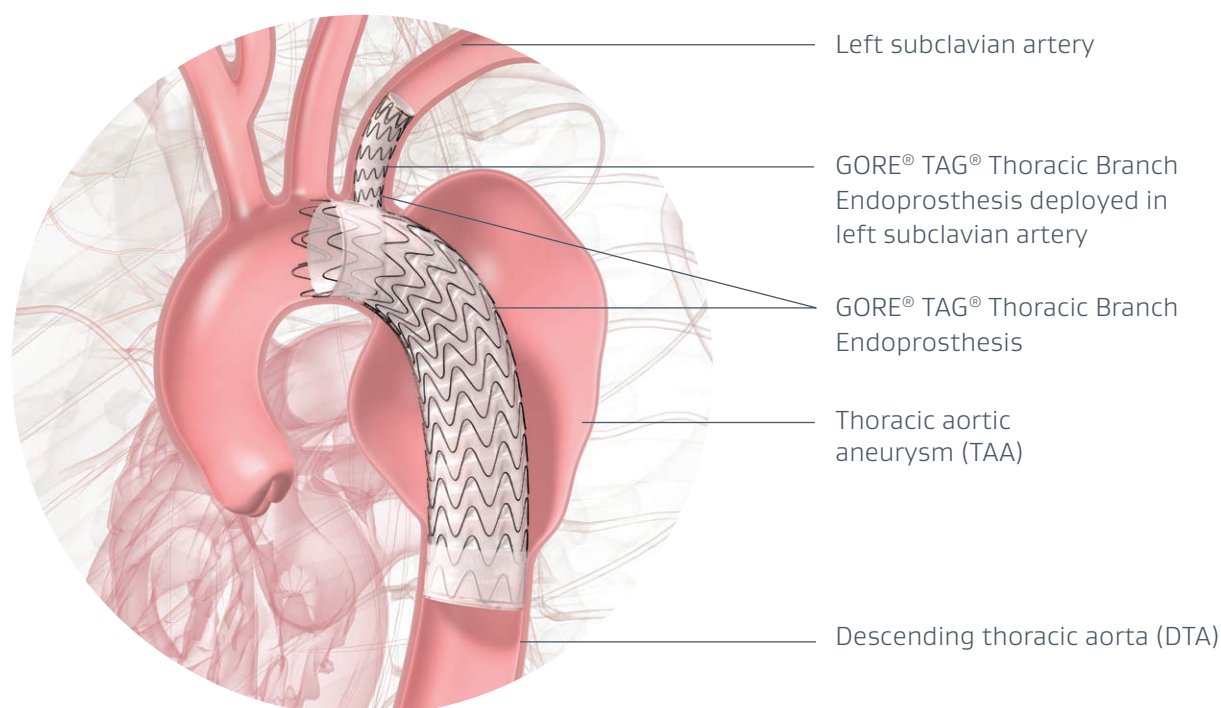


Figure 1. GORE® TAG® Thoracic Branch Endoprosthesis deployed in the left subclavian artery and the descending thoracic aorta.

* Refer to *Instructions for Use* at elfu.goremedical.com for a complete description of all applicable indications, warnings, precautions and contraindications for the markets where this product is available. Rx Only

Table 1: Centers for Medicare and Medicaid Services (CMS) Fiscal Year 2024 Medicare Severity Diagnosis Related Groups (MS-DRGs)

The following MS-DRGs are the most commonly assigned for the TBE procedure. Other DRGs may apply based on documented procedures performed, patient’s condition or complications.

Medicare Inpatient Prospective Payment System (IPPS)			
MS-DRGs	Description	Relative weight	Medicare national unadjusted amount
219	Cardiac valve and other major cardiothoracic procedures without cardiac catheterization with major complication or comorbidity (MCC)	7.7112	\$53,990.74
220	Cardiac valve and other major cardiothoracic procedures without cardiac catheterization with complication or comorbidity (CC)	5.2446	\$36,720.59
221	Cardiac valve and other major cardiothoracic procedures without cardiac catheterization without CC/MCC	4.6486	\$32,547.64

Reference: [FY 2024 IPPS Final Rule Home Page | CMS](#)

Table 2: International Classification of Diseases (ICD)-10-PCS

TBE must be reported with both of the assigned ICD-10-PCS codes below.
Code all other procedures documented applicable to case.

ICD-10-PCS	Description
02VW3DZ	Restriction of thoracic aorta, descending with intraluminal device, percutaneous approach
02VX3EZ	Restriction of thoracic aorta, ascending/arch with branched or fenestrated intraluminal device, one or two arteries, percutaneous approach

Reference: [2024 ICD-10-PCS | CMS](#)

CPT Copyright 2024 American Medical Association. All rights reserved.
CPT® is a registered trademark of the American Medical Association.

Table 3: Current procedural terminology (CPT®) code

Surgery/cardiovascular system

Miscellaneous code 33999 should be utilized to report TBE procedure in absence of a descriptive code.
Code with all other interventions applicable.

Healthcare common procedure coding system (HCPCS)	Description	Pro fee facility total relative value units (RVUs)	Pro fee facility adjusted partial payment
33999	Unlisted procedure, cardiac surgery	0.00	\$0.00

Comparator equals previous surgical procedural coding RVU for reporting purposes.
Individual payors contractual terms may differ according to miscellaneous code usage.
Gore suggests contacting and following payor contractual agreements for reporting purposes.

New Technology Add-on Payment (NTAP)^{*,†}

The Centers of Medicare & Medicaid Services (CMS) created the NTAP to help ensure hospitals do not incur significant reimbursement shortfalls when adopting innovative new technologies. NTAP is additional payment on top of the Medicare Severity Diagnosis Related Group (MS-DRG) or TRICARE[®] DRG reimbursement.

Approval granted:

- Cost criterion: Cost for cases involving TBE “exceeds the case-weighted threshold amount.”
- FDA marketing authorization May 13, 2022, for indication covered by its Breakthrough Device designation for endovascular repair of lesions of the descending thoracic aorta, while maintaining flow into the left subclavian artery, in patients who are at high risk for debranching subclavian procedures and have appropriate anatomy.[‡]

Reporting add-on payment:

The International Classification of Diseases 10th Revision Procedure Coding System (ICD-10-PCS) code for reporting will be effective October 1, 2022. Hospitals can report the codes on claim forms for procedures[‡] related to TBE to receive the add-on payment for eligible inpatient cases.

Details of the NTAP:

Eligible facilities	Acute care hospitals participating in the inpatient prospective payment system (IPPS) are eligible. Hospitals under the TRICARE [®] program are eligible.
Qualified patients	Traditional Medicare and dual-eligible (Medicare-Medicaid) fee-for-service patients or TRICARE [®] patients whose case totals exceed the MS-DRG rate payment are qualified.
Add-on payment	NTAP is limited to lesser of 65% of the cost of the new technology or 65% of the amount by which the cost of case exceeds the MS-DRG payment.
Payment amount	Total \$27,807 per maximum amount. Effective October 1, 2022.
Duration	NTAP is approved for a minimum of two years and no more than three years; the maximum add-on payment amount is reassessed annually.
Coding requirements	ICD-10-PCS Codes: (Both must be reported on claim) ² 02VX3EZ – Restriction of thoracic aorta, ascending/arch with branched or fenestrated intraluminal device, one or two arteries, percutaneous approach. 02VW3DZ – Restriction of thoracic aorta, descending with intraluminal device, percutaneous approach.

Exclusion criteria:

- Hospitals not reimbursed under the IPPS – (Include but not limited to critical access hospitals, excluded cancer hospitals, long-term acute care hospitals, Veterans Affairs [VA] hospitals, Department of Defense [DoD] facilities and hospitals in the state of Maryland are not eligible to receive add-on payments).

* Outlier payments are still applicable when eligible and all payments vary by hospital and are case-dependent.
<https://www.cms.gov/Medicare/Medicare-Fee-for-Service-Payment/AcuteInpatientPPS/outlier>

† Refer to *Instructions for Use* at eifu.goremedical.com for a complete description of all applicable indications, warnings, precautions and contraindications for the markets where this product is available. ^{Rx Only}

‡ Hospitals remain responsible for determining correct coding and reimbursement reporting.

TRICARE is a trademark of the Department of Defense (DoD), Defense Health Agency (DHA).

Sample CMS-1450 (UB04) claim form ^{*,†,3}

The information below refers to the paper format of the CMS-1450 (UB-04). Providers submitting claims for TBE via electronic software systems are urged to translate claim information into compatible formats for input into their software system.


1		2		3a PAT. CNTRL. # b. MED. REC. #		4 TYPE OF BILL	
5 FED. TAX NO.		6 STATEMENT COVERS PERIOD FROM		7 THROUGH			
8 PATIENT NAME		a		9 PATIENT ADDRESS		a	
10 BIRTHDATE		11 SEX		12 DATE		13 ADMISSION 13 HR 14 TYPE 15 SRC 16 DHR 17 STAT	
18		19		20		21	
22		23		24		25	
26		27		28		29 ACCT STATE	
30		31		32		33	
34		35		36		37	
38		39		40		41	
42		43		44		45	
46		47		48		49	
50		51		52		53	
54		55		56		57	
58		59		60		61	
62		63		64		65	
66		67		68		69	
70		71		72		73	
74		75		76		77	
78		79		80		81	
82		83		84		85	
86		87		88		89	
90		91		92		93	
94		95		96		97	
98		99		100		101	
102		103		104		105	
106		107		108		109	
110		111		112		113	
114		115		116		117	
118		119		120		121	
122		123		124		125	
126		127		128		129	
130		131		132		133	
134		135		136		137	
138		139		140		141	
142		143		144		145	
146		147		148		149	
150		151		152		153	
154		155		156		157	
158		159		160		161	
162		163		164		165	
166		167		168		169	
170		171		172		173	
174		175		176		177	
178		179		180		181	
182		183		184		185	
186		187		188		189	
190		191		192		193	
194		195		196		197	
198		199		200		201	
202		203		204		205	
206		207		208		209	
210		211		212		213	
214		215		216		217	
218		219		220		221	
222		223		224		225	
226		227		228		229	
230		231		232		233	
234		235		236		237	
238		239		240		241	
242		243		244		245	
246		247		248		249	
250		251		252		253	
254		255		256		257	
258		259		260		261	
262		263		264		265	
266		267		268		269	
270		271		272		273	
274		275		276		277	
278		279		280		281	
282		283		284		285	
286		287		288		289	
290		291		292		293	
294		295		296		297	
298		299		300		301	
302		303		304		305	
306		307		308		309	
310		311		312		313	
314		315		316		317	
318		319		320		321	
322		323		324		325	
326		327		328		329	
330		331		332		333	
334		335		336		337	
338		339		340		341	
342		343		344		345	
346		347		348		349	
350		351		352		353	
354		355		356		357	
358		359		360		361	
362		363		364		365	
366		367		368		369	
370		371		372		373	
374		375		376		377	
378		379		380		381	
382		383		384		385	
386		387		388		389	
390		391		392		393	
394		395		396		397	
398		399		400		401	
402		403		404		405	
406		407		408		409	
410		411		412		413	
414		415		416		417	
418		419		420		421	
422		423		424		425	
426		427		428		429	
430		431		432		433	
434		435		436		437	
438		439		440		441	
442		443		444		445	
446		447		448		449	
450		451		452		453	
454		455		456		457	
458		459		460		461	
462		463		464		465	
466		467		468		469	
470		471		472		473	
474		475		476		477	
478		479		480		481	
482		483		484		485	
486		487		488		489	
490		491		492		493	
494		495		496		497	
498		499		500		501	
502		503		504		505	
506		507		508		509	
510		511		512		513	
514		515		516		517	
518		519		520		521	
522		523		524		525	
526		527		528		529	
530		531		532		533	
534		535		536		537	
538		539		540		541	
542		543		544		545	
546		547		548		549	
550		551		552		553	
554		555		556		557	
558		559		560		561	
562		563		564		565	
566		567		568		569	
570		571		572		573	
574		575		576		577	
578		579		580		581	
582		583		584		585	
586		587		588		589	
590		591		592		593	
594		595		596		597	
598		599		600		601	
602		603		604		605	
606		607		608		609	
610		611		612		613	
614		615		616		617	
618		619		620		621	
622		623		624		625	
626		627		628		629	
630		631		632		633	
634		635		636		637	
638		639		640		641	
642		643		644		645	
646		647		648		649	
650		651		652		653	
654		655		656		657	
658		659		660		661	
662		663		664		665	
666		667		668		669	
670		671		672		673	
674		675		676		677	
678		679		680		681	
682		683		684		685	
686		687		688		689	
690		691		692		693	
694		695		696		697	
698		699		700		701	
702		703		704		705	
706		707		708		709	
710		711		712		713	
714		715		716		717	
718		719		720		721	
722		723		724		725	
726		727		728		729	
730		731		732		733	
734		735		736		737	
738		739		740		741	
742		743		744		745	
746		747		748		749	
750		751		752		753	
754		755		756		757	
758		759		760		761	
762		763		764		765	
766		767		768		769	
770		771		772		773	
774		775		776		777	
778		779		780		781	
782		783		784		785	
786		787		788		789	
790		791		792		793	
794		795		796		797	
798		799		800		801	
802		803		804		805	
806		807		808		809	
810		811		812		813	
814		815		816		817	
818		819		820		821	
822		823		824		825	
826		827		828		829	
830		831		832		833	
834		835		836		837	
838		839		840		841	
842		843		844		845	
846		847		848		849	
850		851		852		853	
854		855		856		857	
858		859		860		861	
862		863		864		865	
866		867		868		869	
870		871		872		873	
874		875		876		877	
878		879		880		881	
882		883		884		885	
886		887		888		889	
890		891		892			

Procedural steps


The procedure for implanting the GORE® TAG® Thoracic Branch Endoprosthesis consists of the delivery of the stent grafts into the aorta and the left subclavian artery. While the endovascular procedure is similar for trauma or dissection repair, below is an example of the steps included in an aneurysm repair.

The main body stent graft is implanted using fluoroscopy, or real-time X-ray images, and is viewed on a monitor following these steps:


1. The delivery catheter, which contains the stent graft, is inserted into the femoral or iliac artery and carefully guided through the abdomen into the chest to the site of the diseased or injured aorta.
2. Once the stent graft is correctly positioned in the aorta and aligned with the left subclavian artery, it is released, or deployed, from the delivery catheter. The device self-expands to the diameter of the aorta and the delivery catheter is withdrawn from the body.
3. A second, smaller stent graft is inserted into the femoral or iliac artery and positioned through the opening of the first stent graft into the left subclavian artery.
4. Once the second stent graft is correctly positioned within the left subclavian artery, it is released, or deployed, from the delivery catheter. The delivery catheter is then removed.
5. Following deployment, an endovascular balloon may be inflated inside the device to aid the device in opening completely, allowing the device to achieve better seal.

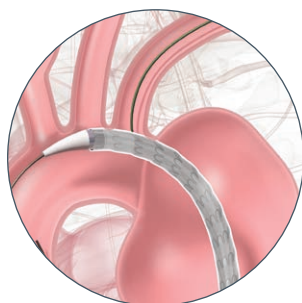


Positioning aortic component at left subclavian artery

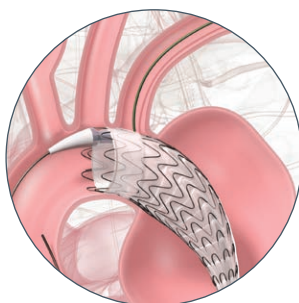

Deployment of aortic component

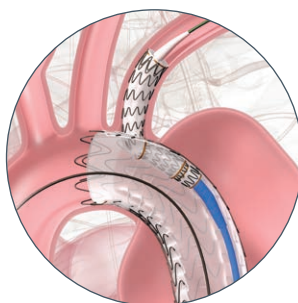

Positioning of side branch component into left subclavian artery

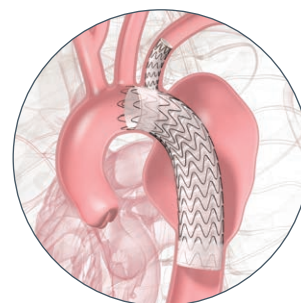

Final GORE® TAG® Thoracic Branch Endoprosthesis system

In some cases, it may be necessary to utilize an additional component(s) to extend proximal into the aortic arch or distal into the descending aorta. Physicians determine the actual devices utilized based on individual patient needs.

References

1. Department of Health & Human Services. Centers for Medicare & Medicaid Services (CMS), Department of Health and Human Services (HHS). Medicare Program; Hospital Inpatient Prospective Payment Systems for Acute Care Hospitals and the Long-Term Care Hospital Prospective Payment System and Policy Changes and Fiscal Year 2024 Rates; Quality Programs and Medicare Promoting Interoperability Program Requirements for Eligible Hospitals and Critical Access Hospitals; Costs Incurred for Qualified and Non-Qualified Deferred Compensation Plans; and Changes to Hospital and Critical Access Hospital Conditions of Participation. A Rule by the Centers for Medicare & Medicaid Services on 08/10/2022. *Federal Register* 2022;87(153):48780-49499. <https://www.govinfo.gov/content/pkg/FR-2023-08-28/pdf/2023-16252.pdf>
2. U.S. Centers for Medicare & Medicaid Services. 2024 ICD-10 Procedure Coding System (ICD-10-PCS). Updated May 26, 2022. Accessed November 4, 2022. <https://www.cms.gov/medicare/coding-billing/icd-10-codes/2024-icd-10-pcs>
3. National Uniform Billing Committee (NUBC). Billing information. American Hospital Association. Accessed November 4, 2022. <https://www.nubc.org/>
4. U.S. Centers for Medicare & Medicaid Services. 2022 ICD-10 Procedure Coding System (ICD-10-PCS). Updated 01/12/2022. Accessed November 4, 2022. <https://www.cms.gov/medicare/icd-10/2022-icd-10-pcs>

For coding and/or reimbursement support, contact:

REVENUE CYCLE CODING STRATEGIES® (RCCS) at +1 888 812 0322 or visit goremedical.com/coding



INDICATIONS FOR USE IN THE U.S.: The GORE® TAG® Thoracic Branch Endoprosthesis is indicated for endovascular repair of lesions of the descending thoracic aorta, while maintaining flow into the left subclavian artery and have: **Adequate iliac/femoral access; Proximal Aortic Landing Zones:** For Isolated Lesion Patients: Proximal landing zone cannot be aneurysmal, dissected, heavily calcified or heavily thrombosed; For Dissection Patients: Primary entry tear must be distal to the left subclavian artery and the proximal extent of the landing zone must not be dissected; Aortic inner diameter range 16–42 mm; Proximal segment length (length from distal edge of left subclavian artery to mid left common carotid ostium) of at least 2.0–4.0 cm, depending on Aortic Component selection; Proximal covered length (measured from distal edge of left subclavian artery to distal edge of left common carotid artery ostium) of at least 15–36 mm, depending on Aortic Component selection; For patients with prior ascending aorta or aortic arch repair with surgical graft: at least 2 cm landing zone proximal to the distal anastomosis; **Left Subclavian Landing Zone:** Landing zone cannot be aneurysmal, dissected, heavily thrombosed and severely tortuous (180 degree turn within the treated length); Left subclavian artery inner diameter of 6–18 mm, depending on Side Branch Portal diameter selected; Left subclavian artery minimum length of 2.5–3.0 cm, depending on Side Branch Portal diameter selected. **Distal Landing Zone (Isolated Lesion Patients only):** Outer curve length must be ≥ 2 cm proximal to celiac artery; Aortic inner diameter range 16–42 mm; Non aneurysmal, dissected, heavily calcified or heavily thrombosed landing zone; Native Aorta or previously placed GORE® TAG® Conformable Thoracic Stent Graft.

CONTRAINDICATIONS: The GORE® TAG® Thoracic Branch Endoprosthesis is contraindicated in: Patients with known sensitivities or allergies to the device materials [ePTFE (polytetrafluoroethylene), FEP (fluoroethylpropylene), Nitinol (nickel, titanium), Gold, SB Component only - Heparin (CBAS® Heparin Surface)]; Patients who have a condition that threatens to infect the graft; Patients with known hypersensitivity to heparin, including those patients who have had a previous incident of Heparin-Induced Thrombocytopenia (HIT) type II. Refer to *Instructions for Use* at eifu.goremedical.com for a complete description of all applicable indications, warnings, precautions and contraindications for the markets where this product is available. ^{Rx Only}

Products listed may not be available in all markets.

CPT® is a registered trademark of the American Medical Association (AMA). Copyright 2024 AMA. All rights reserved.

TRICARE is a trademark of the Department of Defense (DoD), Defense Health Agency (DHA).

REVENUE CYCLE CODING STRATEGIES is a trademark of Revenue Cycle Coding Strategies, LLC.

CBAS is a trademark of Carmeda AB, a wholly owned subsidiary of W. L. Gore & Associates, Inc.

GORE, *Together, improving life*, TAG and designs are trademarks of W. L. Gore & Associates.

© 2022, 2023 W. L. Gore & Associates, Inc. 231206902-EN OCTOBER 2023

W. L. Gore & Associates, Inc.
goremedical.com

Asia Pacific +65 67332882 Australia/New Zealand 1800 680 424 Europe 00800 6334 4673
United States Flagstaff, AZ 86004 800 437 8181 928 779 2771

