



# NEW PRODUCT FOR ABDOMINAL WALL RECONSTRUCTION

## GORE® ENFORM Biomaterial

- Optimal handling
- Infiltration to enable vascularization
- Regeneration to leave only healthy tissue

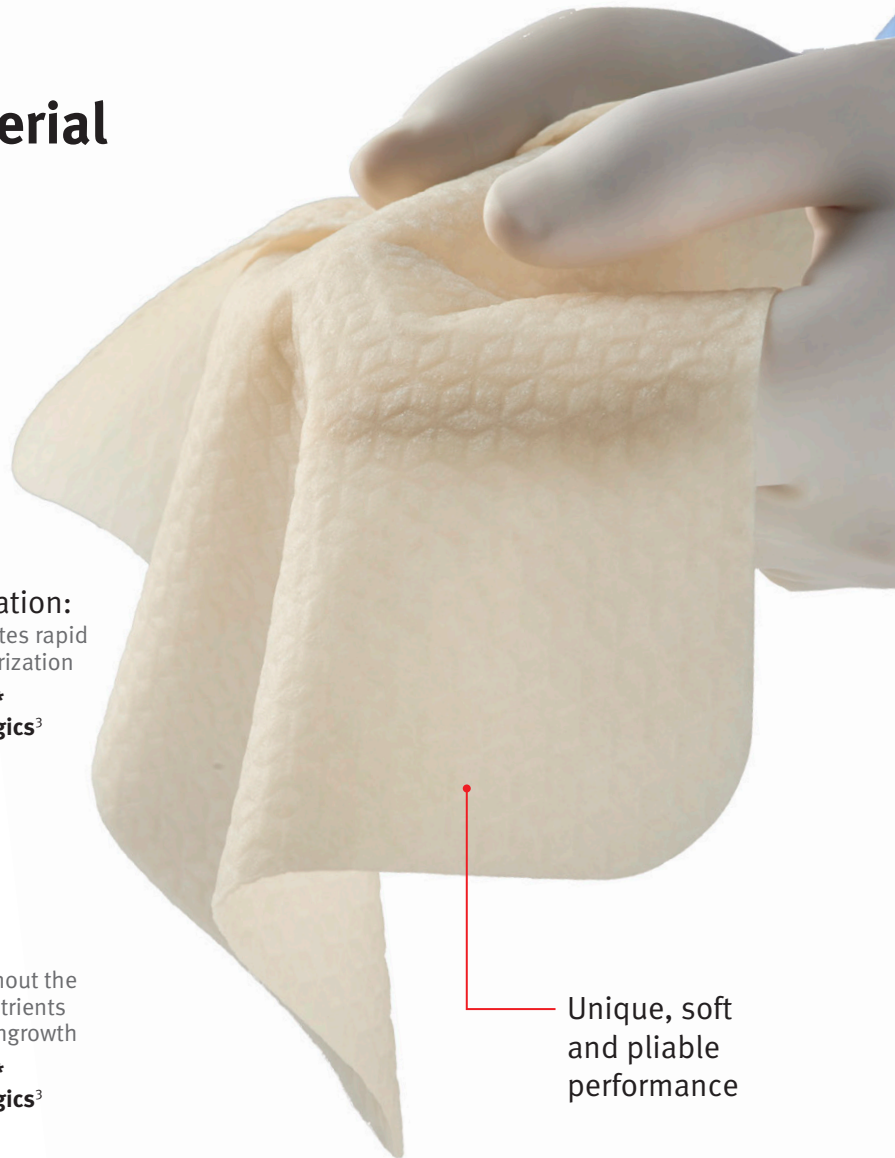


Unique, soft and pliable performance

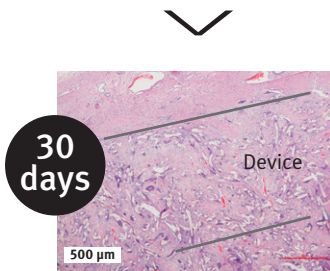

### INFILTRATION

to enable vascularization:  
Optimal pore size<sup>1,2</sup> facilitates rapid cell infiltration and vascularization


**2X fibrous tissue ingrowth\* compared to popular biologics<sup>3</sup>**

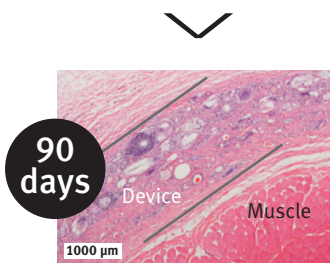

### INTEGRATION

to support healthy tissue formation:  
Vascularized tissue throughout the matrix delivers cells and nutrients to the site for rapid tissue ingrowth

**3X fibrous tissue ingrowth\* compared to popular biologics<sup>3</sup>**

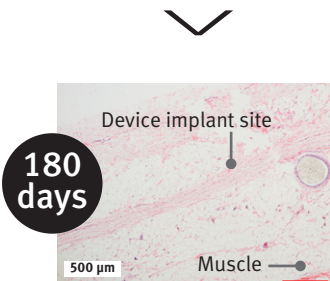

### REGENERATION

to leave only healthy tissue:  
Uniform collagen replaces the bioabsorbable matrix


**Uniform, mature collagen replaces the bioabsorbable matrix<sup>4</sup>**



## FEEL THE CONFORMABILITY


Contact your Gore Sales Associate to experience the difference.

## Configurations for preperitoneal placement

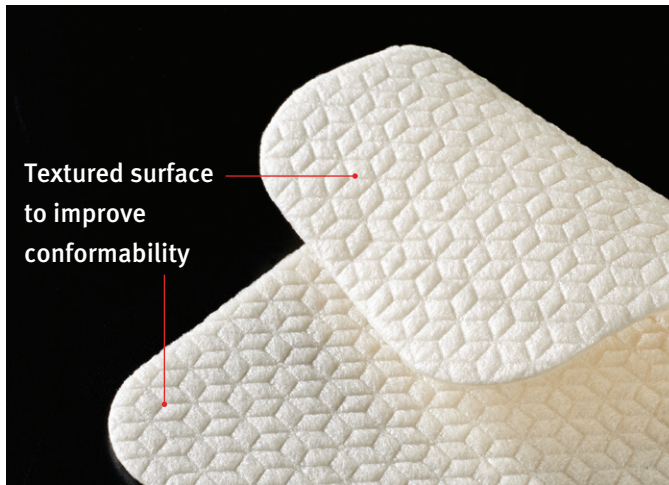

Catalogue Number	Dimensions (cm x cm)
GBWR0616	6 x 16
GBWR0816	8 x 16
GBWR1010	10 x 10
GBWR1016	10 x 16
GBWR1620	16 x 20
GBWR2020	20 x 20
GBWR2025	20 x 25
GBWR2030	20 x 30
GBWR2040	20 x 40
GBWR2540	25 x 40
GBWR3030	30 x 30
GBWR3040	30 x 40

## Configurations for intraperitoneal placement

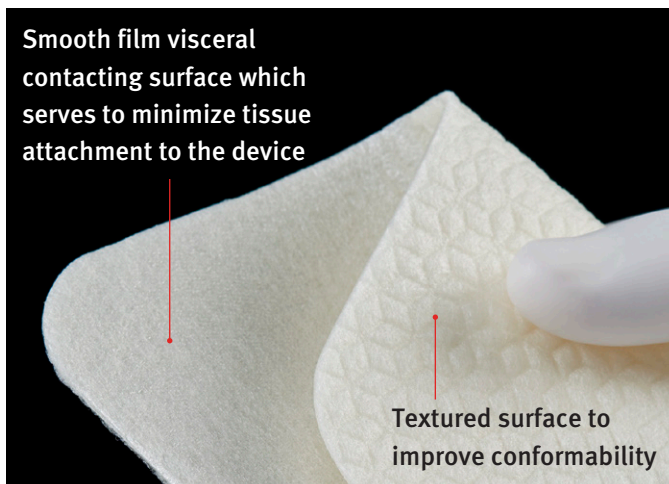

Catalogue Number	Dimensions (cm x cm)
GBFR0816	8 x 16
GBFR1016	10 x 16
GBFR1620	16 x 20
GBFR2025	20 x 25
GBFR2540	25 x 40

Both the textured ingrowth surface and the smooth FILM surface are comprised of synthetic absorbable (polyglycolic acid: trimethylene carbonate) copolymer (PGA:TMC).



**W. L. GORE & ASSOCIATES, INC.**

Flagstaff, AZ 86004

+65.67332882 (Asia Pacific) 800.437.8181 (United States)  
00800.6334.4673 (Europe) 928.779.2771 (United States)

[goremedical.com](http://goremedical.com)

\* Results may not correlate to clinical performance in humans.

- Sharkawy AA, Klitzman B, Truskey GA, Reichert WM. Engineering the tissue which encapsulates subcutaneous implants. II. Plasma-tissue exchange properties. *Journal of Biomedical Materials Research* 1998;40(4):586-597.
- Rosengren A, Bjursten LM. Pore size in implanted polypropylene filters is critical for tissue organization. *Biomedical Materials Research. Part A*. 2003;67(3):918-926.
- Sanchez R, Crawford N. *Tissue Characterization of GORE TRX, STRATTICE™ Reconstructive Tissue Matrix, XenMatrix™ Surgical Graft and Phasix ST™ Mesh in a subcutaneous rabbit model at 30 and 90 days*. Flagstaff, AZ: W. L. Gore & Associates, Inc.; 2018. [Study protocol]. 24665C.
- Sanchez R, Crawford N. *Tissue Characterization of GORE TRX, STRATTICE™ Reconstructive Tissue Matrix, XenMatrix™ Surgical Graft and Phasix ST™ Mesh in a subcutaneous rabbit model at 180 days*. Flagstaff, AZ: W. L. Gore & Associates, Inc.; 2018. [Study protocol]. 24675C.

Products listed may not be available in all markets.