


血液透析人工血管动静脉瘘 护理及穿刺技术



PERFORMANCE through innovation

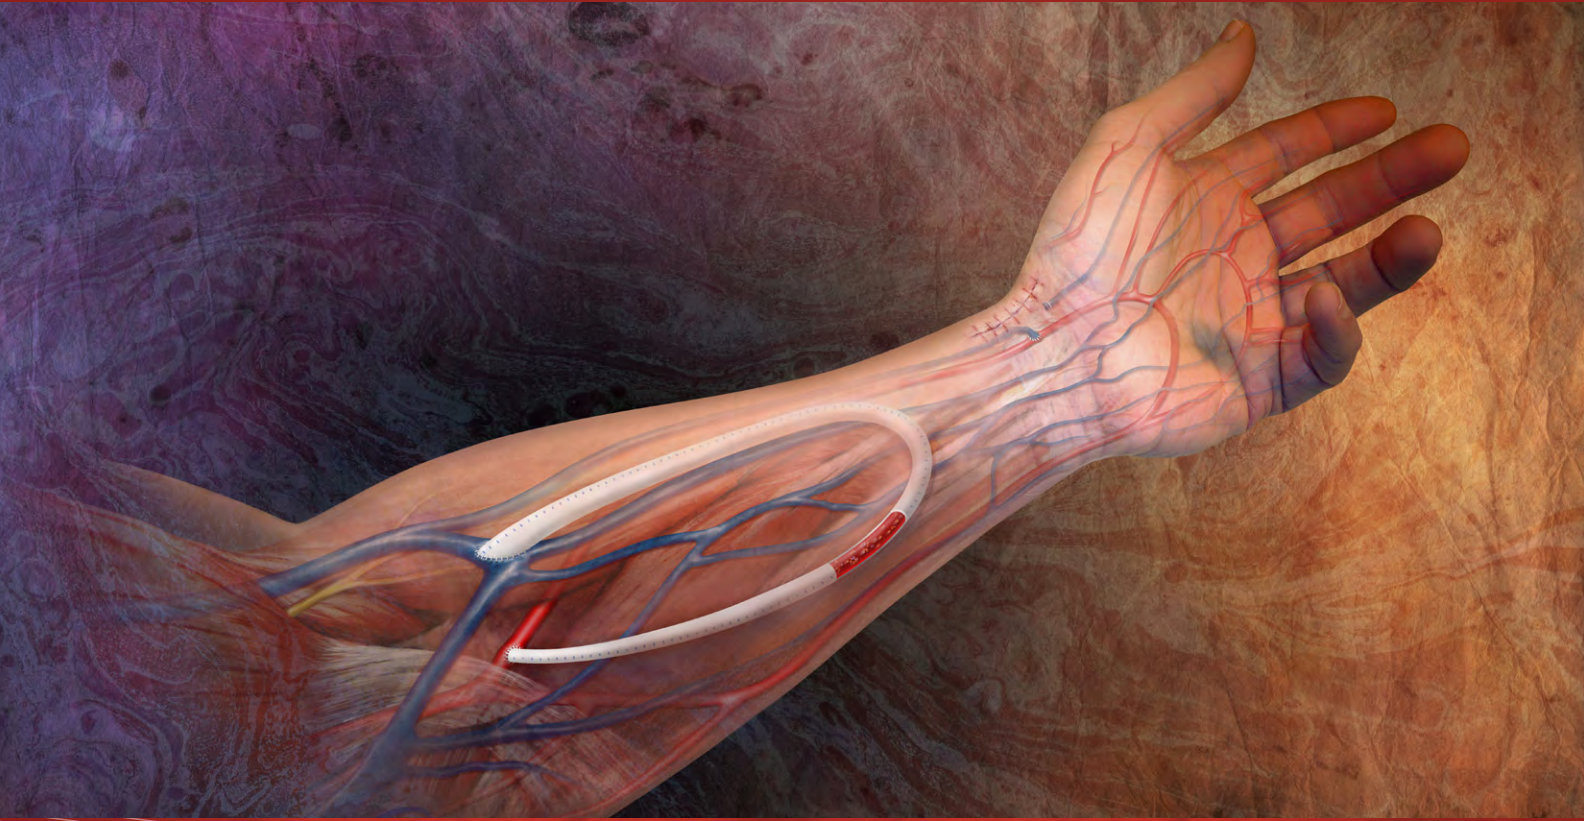

戈尔（GORE）血液透析人工血管：护理及穿刺技术



血液透析患者的长期支持治疗需要安全有效的穿刺动静脉瘘，这对于以戈尔（GORE）人工血管动静脉瘘作为透析通路的患者也十分重要。透析护士在相当大的程度上担负着确保充分透析的责任。尽管患者个人情况和透析中心设备都各不相同，但是从各主要透析中心多年所积累的经验中，已经证实了一些有益的人工血管穿刺技术。坚持使用这些技术有助于提高人工血管动静脉瘘的使用寿命并改善患者的生活质量。此外，穿刺进度也会更快、问题更少，从而提高透析室的整体效率。

！ 人工血管

在30多年的应用中，戈尔（Gore）人工血管始终能战胜最苛刻的血管手术难题的挑战。凭借公认的优异性能和质量，赢得了全球知名外科医生的青睐。这些人工血管无需预凝处理、抗膨胀并能够防止感染扩散，并最大程度保障血栓切除术的安全。Gore人工血管具有多种规格型号，包括延展性及非延展性，直型、锥型及分叉型等构型，以及由外环支撑或一体式内环径向支撑的结构。

GORE人工血管的穿刺

在手术植入Gore人工血管后，医生通常要求等待几周后才能进行穿刺。患者愈合情况各有不同，但在这段时间内，组织充分生长进入人工血管外壁，使人工血管得以固定。这对于预防感染和血肿至关重要。

在某些情况下，医生可能会建议患者在没有完全愈合之前接受血液透析。在此，对于这些患者的护理工作必须极为小心，[参见早期穿刺特别注意事项部分]。只有在别无他选的情况下，才能考虑进行立即或提早人工血管穿刺。



人工血管动静脉瘘评估

人工血管穿刺前的愈合期

患者的人工血管良好愈合后，穿刺部位的检查即成为每次透析时的常规步骤。感染、血肿和假性动脉瘤会引发诸多问题，使穿刺变得十分困难，甚至十分危险。早期发现这些问题并及时告知医生可以保护人工血管甚至拯救患者的生命。最严重的并发症包括：

- 感染
- 假性动脉瘤
- 血肿



感染

穿刺部位出现感染的表现有局部肿胀、发红、疼痛和流脓。如果出现这些或其他可疑症状，应立即通知医生。**切勿在感染区域入针。**因为这样，会直接将细菌引入到血液中。严格遵守无菌技术可显著减少感染的几率[参见无菌操作部分]。



假性动脉瘤

假性动脉瘤，是指血液漏出人工血管并被周围组织包裹而形成的血肿。这种血液渗漏主要由两个因素造成。在同一部位反复穿刺破坏了人工血管的完整性，以及静脉吻合口或流出道狭窄导致人工血管内的压力升高。¹这种压力可能会迫使血流通过人工血管上的穿刺针孔流入血管周边组织，从而导致假性动脉瘤。为了阻止假性动脉瘤增大，必须对所有静脉流出道的显著狭窄部位实施经皮腔内血管成形术（PTA）。对病变部分成功实施PTA可以减少人工血管内压力，减少进入假性动脉瘤的血流量。

假性动脉瘤的进行性增大可能会导致穿刺困难并且在拔针时难以止血。假性动脉瘤增大的其他并发症包括被覆皮肤破裂、自发性出血和急性假性动脉瘤囊破裂。人工血管感染的几率也会增大。²

在同一部位反复穿刺（“一处多穿”）或“穿刺处撕裂（病变）”，都会导致假性动脉瘤。沿着整个人工血管的长度进行轮换穿刺是至关重要的，可谓重中之重。



人工血管“一处多穿”部位。



血肿

血肿是人工血管穿刺部位出血未得到控制的结果。血液在组织和人工血管壁之间扩散开来，导致肿胀和变色。请勿通过血肿部位穿刺。因为穿刺针通常会凝血，从而需要在一个新部位穿刺人工血管。而且，在穿刺失败的位置必须施以压力以防止血肿扩大，因而使穿刺难度增大。同时也会使得可穿刺位置减少。


根据血肿的严重性，请及时咨询医生，清除血肿并纠正血肿出现的原因。穿刺期间和之后，谨慎的操作将大大降低血肿的发生率[参见穿刺技术部分]。

检查人工血管的血流量

在任何时间，如果人工血管的血流量降低，不仅会加大血液导入透析机的难度，还可能造成人工血管闭塞的情况。要检查管腔内是否有足够的血流，可以触诊整个人工血管是否有强烈“震颤”。震颤的手感是皮下的持续振动，而不是脉搏跳动的感觉。有跳动感的搏动表明在血液通路中存在着狭窄处。血管震颤则表明血流量充足。

如果不能触摸到震颤，可以用听诊器听辨血液快速流过人工血管时的声音，或“杂音”。这两者在强度和性质上的变化都应该记录在患者病历表上。如果没有震颤或者杂音，请勿进行穿刺。

了解透析人工血管内的血流方向也十分重要。静脉针应与血流方向相同。这样可以防止出现再循环，并有助于静脉回流处于正常状态。在理想情况保持下，外科医生应提供一张示意图用以说明人工血管的位置和血液流动的方向。如果没有示意图，您可以使用下面这个简单方法来判断血流方向。

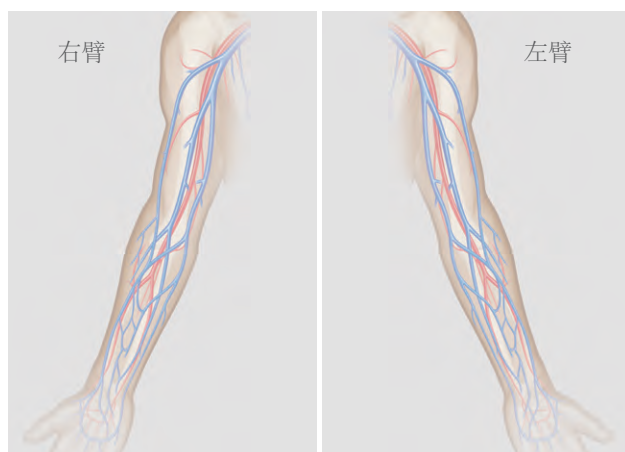

透析穿刺计划表

用手指对人工血管中部施加短暂的压力，并触诊人工血管的震颤。脉动最强的一边就是血液进入人工血管的方向，即动脉侧。

针具选择

应使用能够达到透析机所需流量的最小尺寸的针具。因此，超薄壁带背孔针是很好的选择。针的长度则因人工血管在组织中的深度不同而异。在大多数情况下，一英寸长的针是适宜的，有助于减少损坏人工血管后壁的几率。一般来讲，总是选择适合患者的最小最短的针具。

评估人工血管动静脉瘘

使用透析穿刺计划图表来标出穿刺位置和日期有助于纪录已用的穿刺部位并且避免“一处多穿”。穿刺位置应该在人工血管的直行部分，并且应远离人工血管与动脉或静脉缝合处至少三厘米。穿刺点之间应保持一厘米左右的间距。两到三周之后才能从原来穿刺点一厘米以内进行穿刺。

U形人工血管的弧形转弯部分不宜穿刺，因为很难正确定位穿刺针。尤其是如果使用的是有外环的人工血管，这些防止人工血管扭结的外环正处于这个区域，它们的存在可能对穿刺造成额外困难。

! 无菌准备

必须彻底消毒皮肤以减少人工血管感染的几率。实施穿刺应被视为具有污染和感染风险的外科手术。根据各血液透析中心的章程，透析工作人员可自由选择配戴无菌手套。但是，应避免徒手、用非无菌手套或器械或者透析设备接触消毒好的针头穿刺部位。要确保合理使用手术口罩。血液透析患者中，有很高比例（32-81%）在鼻腔中携带有高于正常水平的金黄色葡萄球菌。³

患者在进入透析室时应使用抗菌肥皂和水清洗他们的穿刺部位。在使用抗菌剂前先给予异丙醇有助于清除皮肤上的污垢和油脂。在检查选定的穿刺部位后，用2%的葡萄糖酸氯己定/70%的异丙醇或70%的酒精和/或10%的聚维酮碘清洗选定的部位。⁴



2%葡萄糖酸氯己定/70%异丙醇抗菌剂对皮肤具有快速（30秒）和持久（长达48小时）的抗菌作用。应用该溶液时来回涂擦30秒。等该部位变干。不要擦掉溶液。⁴

酒精能够起到短暂的抑菌作用，应该在进针前揉擦一分钟。⁴

聚维酮碘需要2-3分钟才能充分发挥抑菌作用，必须在其变干后进行穿刺。⁴

穿刺技术

使用两个透析针进行血透时，动脉穿刺针可以顺着血流方向也可逆着血流方向进针。当动脉穿刺针的方向为顺血流方向时，引起的血流湍流比较小。静脉穿刺针（回流）则必须始终顺血流方向进针。如果使用单个透析针进行透析，穿刺针必须始终顺血流方向进针。

沿进针方向相反的方向，绷紧进针处的皮肤。压力不可过大，否则会使得人工血管变平而不易穿刺。[图1]

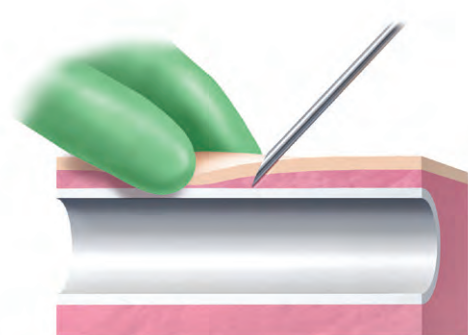


图1

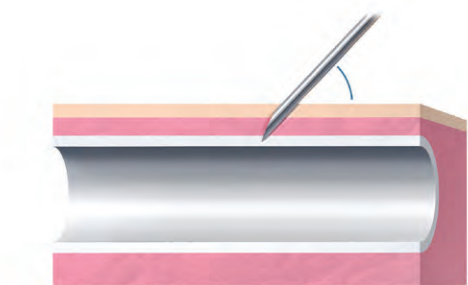


图2



图3

通常，穿刺时针头斜面朝上并按照一定角度刺入皮肤。进针的角度则取决于人工血管的形状，位置和深度 [图2]。

保持理想进针角度，轻轻的将针刺入人工血管壁。 [图3]

固定住人工血管的位置，有利于加强穿刺的准确性。注意观察回血的情况，如果没有回血或者回血缓慢，需确认针尖的位置，可以尝试用注射器灌洗针头及导管。没有回血或者回血缓慢的潜在原因包括：

- 穿刺针斜面抵触人工血管壁
- 针头未完全刺入人工血管
- 针头已穿透人工血管前、后壁
- 患者血压偏低
- 由于 血液透析通路堵塞，人工血管内血流欠佳

确认回血良好后，继续向前推针少许，深度不超过八分之一英寸（约3.2毫米），以确保针尖位于管腔内。



图4

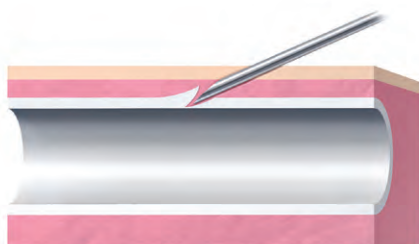


图5

继续进针，直到针座[图4]。此推入过程中，保持穿刺针贴近皮下或者近乎平行于皮肤，有利于避免穿透人工血管后壁。

以约 45° 的角度进针，会在人工血管壁的穿刺部位形成一个活瓣。这个活瓣在拔针时，发挥类似“阀门”的功能以减少穿刺点出血[图5]。

如果平行进针，则有可能损伤人工血管。

随着经验的积累，透析护士/技术人员对于人工血管穿刺将会有获得准确的手感。

在整个穿刺过程中，切勿污染消毒过的穿刺部位。注意观察反常的阻力或者疼痛。一旦穿刺针完全推入并且固定针翼后，患者应该不会感到不适。持续的疼痛有可能表明针头刺入了人工血管后壁，这种情况下，回抽血流往往是缓慢或者不规则的。这些问题必须在继续进行透析之前解决。

透析完成后

透析完成后，应小心拔针，并以指端轻压止血。轻轻按压穿刺针刺入人工血管处比按压刺入皮肤处的止血效果要好。用棉球或者纱布敷在针刺入人工血管的位置并保持适度的压力[图 6]，直到出血停止。通常需要按压10-15分钟以达到止血效果。

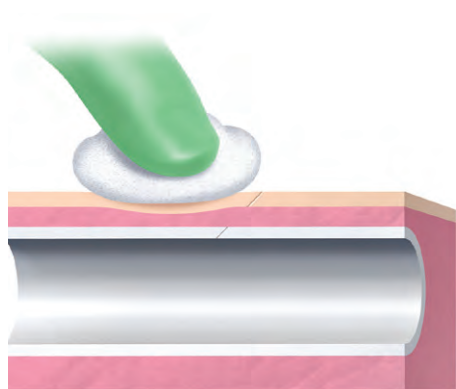


图6

检查穿刺点是否有异常出血的征兆。

在止血时，需要把握压迫的力道。一方面，要施以足够的压力以避免穿刺点出血，另一方面，又要防止压力过大而导致人工血管血栓形成。有时候，根据患者的实际情况，也可用手臂止血夹加压止血。

最后，请在病历上记录穿刺位置和穿刺日期。

早期穿刺的特别注意事项

在特定情况下，医生可能会决定，患者在植入人工血管不久之后就必须接受血液透析治疗。对待这类患者必须格外谨慎，因为出现静脉流出道损伤、血肿和感染的危险很大。

由于术后肿胀，定位人工血管和置入穿刺针会比较困难。穿刺针错位可能会损坏人工血管或穿透人工血管后壁。可用手指轻轻按压来暂时推开肿胀的组织。这样就可以通过触诊或者使用听诊器听辨杂音来确定人工血管的位置。在这些情况下，外科医生所供的示意图就会非常有用。

严格遵守无菌技术是早期穿刺的关键。由于手术切口没有足够的时间充分愈合，建议配戴无菌手套和口罩。

透析完成后，要按压人工血管穿刺部位直到出血停止。通常需要按压10-15分钟以达到止血效果。由于出现了肿胀，患者可能无法对穿刺部位施加充分的压力。

对于人工血管植入后两周内进行透析的情况，一些透析室成功地采用了以下做法：

- 利多卡因局部浸润
- 在穿刺期间防止人工血管移动
- 迅速干净的穿刺
- 小号针头（17号）
- 整个透析过程中保持200-250毫升/分钟的血流量
- 低剂量肝素

提醒列表

- 检查穿刺部位的任何并发症
- 评估人工血管的血流量，并确定血流方向
- 选择尽可能小和短的穿刺针
- 对穿刺部位进行消毒，切勿再接触该部位
- 每次透析更换穿刺部位
- 按照适当的角度穿刺人工血管
- 穿刺时，尽量避免穿透人工血管后壁
- 评估流入和流出穿刺针的血流量是否充足
- 拔针时，需要对人工血管穿刺部位施压非闭塞性的压力，直到出血停止

参考资料和书目

参考文献

1. Vesely TM. Use of stent grafts to repair hemodialysis graft-related pseudoaneurysms. *Journal of Vascular & Interventional Radiology* 2005;16(10):1301-1307
2. National Kidney Foundation DOQI Guidelines. Clinical Practice Guidelines and Clinical Practice Recommendations. Guideline 6. Treatment of arteriovenous graft complications. Graft Degeneration and Pseudoaneurysm Formation (CPG 6.2, CPG 6.3). http://www.kidney.org/professionals/kdoqi/guideline_upHD_PD_VA/va_guide6.htm Published 2006. Accessed August 18, 2011.
3. Boelaert JR, Van Landuyt HW, Gordts BZ, De Baere YA, Messer SA, Herwaldt LA. Nasal and cutaneous carriage of staphylococcus aureus in hemodialysis patients: the effect of nasal mupirocin. *Infection Control & Hospital Epidemiology* 1996;17(12):809-811.
4. National Kidney Foundation DOQI Guidelines. Clinical Practice Guidelines and Clinical Practice Recommendations. Guideline 3. Cannulation of fistulae and grafts and accession of hemodialysis catheters and port catheter systems. http://www.kidney.org/professionals/kdoqi/guideline_upHD_PD_VA/va_guide3.htm Published 2006. Accessed August 18, 2011.

参考书目

Thermann F, Wollert U. Proximalization of the arterial inflow: new treatment of choice in patients with advanced dialysis shunt-associated steal syndrome? *Annals of Vascular Surgery* 2009;23(4):485-490.

Dember LM, Beck GJ, Allon M, et al; Dialysis Access Consortium Study Group. Effect of Clopidogrel on early failure of arteriovenous fistulas for hemodialysis. A randomized controlled trial. *Journal of the American Medical Association* 2008;299(18):2164-2171.

Morsy MA, Khan A, Chemla ES. Prosthetic axillary-axillary arteriovenous straight access (necklace graft) for difficult hemodialysis patients: a prospective single-center experience. *Journal of Vascular Surgery* 2008;48(5):1251-1254.

MacReady N. The D & T Report. The fistula fight. *Dialysis & Transplantation* 2007;36(8):434-435.

Goldin I, Shemesh D, Zaghal I, Berelowitz D, Olsha O. Evaluation of a 6 mm heparin-bonded vascular graft versus standard graft in prosthetic arteriovenous access: first clinical results. Abstract presented at the 5th International Congress of the Vascular Access Society (VAS); June 11-13, 2007; Nice, France. Abstract P-034.

Goldin I, Shemesh D, Zaghal I, Berelowitz D, Olsha O. Evaluation of 6mm heparin-bonded Propaten® graft versus standard graft in prosthetic arteriovenous access—first clinical results. Poster presented at the 5th International Congress of the Vascular Access Society (VAS); June 11-13, 2007; Nice, France.

Kopriva D, Moustapha A. Axillary artery to right atrium shunt for hemodialysis access in a patient with advanced central vein thrombosis: a case report. *Annals of Vascular Surgery* 2006;20(3):418-421.

Besarab A. K/DOQI update. Abstract presented at the 10th Biannual Symposium on Dialysis Access. Vascular Access for Hemodialysis X Symposium; May 18-19, 2006; Phoenix, AZ. Pages 34-43.

Chemla ES. Exotic surgery. Abstract presented at the 10th Biannual Symposium on Dialysis Access. Vascular Access for Hemodialysis X Symposium; May 18-19, 2006; Phoenix, AZ. Page 85.

Lurie DK. Disease management teams for enhancement of graft survival in patients undergoing hemodialysis. Abstract presented at the 10th Biannual Symposium on Dialysis Access. Vascular Access for Hemodialysis X Symposium; May 18-19, 2006; Phoenix, AZ. Page 94-96.

Chemla ES, Morsy M, Anderson L, Makinjuola D. Complex bypasses and fistulas for difficult hemodialysis access: a prospective, single-center experience. *Seminars in Dialysis* 2006;19(3):246-250.

Davidson IJA, Bartsch CC, Bravo K, Gable D, Munschauer C. Stretch expanded polytetrafluoroethylene graft with intrawall radial support system: an advance in vascular access graft design. *Journal of Vascular Access* 2004;5(3):93-98.

Papalois VE, Haritopoulos KN, Labruzzo C, Farrington K, Hakim NS. Reversal of steal syndrome following creation of arteriovenous fistula by banding with a Gore-Tex cuff: a new technique. *International Surgery* 2001;86(4):210-212.

Dolmatch B. Pro/Con - The magic bullet? The best solution for AV graft restenosis so far. Presented at the Controversies in Dialysis Access Meeting; December 8-10, 2005; Scottsdale, AZ. *Journal of Vascular Access* 2005;6(3):124-126.

Saad TF. Pro/Con - The magic bullet? Too early to tell. Presented at the Controversies in Dialysis Access Meeting; December 8-10, 2005; Scottsdale, AZ. *Journal of Vascular Access* 2005;6(3):126-127.

Schild AF, Baltodano NM, Alfieri K, Livingstone J, Raines JK. Pro/Con - Fistula first. Better AV grafts now: improved surgical techniques and graft conduits that all surgeons should know about. Presented at the Controversies in Dialysis Access Meeting; December 8-10, 2005; Scottsdale, AZ. *Journal of Vascular Access* 2005;6(3):143-147.

Peden EK. Pro/Con - 1997 DOQI access guidelines. Five things it got wrong. Presented at the Controversies in Dialysis Access Meeting; December 8-10, 2005; Scottsdale, AZ. *Journal of Vascular Access* 2005;6(3):149-150.

Chemla ES, Korrakuti L, Mankanjuola D, Chang RW. Vascular access in hemodialysis patients with central venous obstruction or stenosis: one center's experience. *Annals of Vascular Surgery* 2005;19(5):692-698.

Thibodeaux LC, Reyes AA. Initial experience with an intrawall, radially supported expanded polytetrafluoroethylene graft for vascular access. In: Henry ML, ed. *Vascular Access for Hemodialysis -IX*. Los Angeles, CA: W.L. Gore & Associates, Inc. & Bonus Books, Inc; 2005:19:195-201.

Davidson IJA, Brava K, Munschauer C, Nichols D, Frawley WH. Conversion of failed native vein fistulas to PTFE grafts yields 90% access function at one year. In: Henry ML, ed. *Vascular Access for Hemodialysis -IX*. Los Angeles, CA: W.L. Gore & Associates, Inc. & Bonus Books; 2005:20:203-206.

Rooijens PPGM, Burgmans JJP, Yo TI, et al. Autogenous radial-cephalic or prosthetic brachial-antecubital forearm loop AVF in patients with compromised vessels? A randomized, multicenter study on the patency of primary hemodialysis access. *Journal of Vascular Surgery* 2005;42(3):481-487.

Bünger CM, Kröger J, Kock L, Henning A, Klar E, Schareck W. Axillary-axillary interarterial chest loop conduit as an alternative for chronic hemodialysis access. *Journal of Vascular Surgery* 2005;42(2):290-295.

Thibodeaux LC, Reyes AA. Initial experience with an intrawall, radially supported ePTFE graft for vascular access. Abstract presented at the 9th Biennial Symposium on Dialysis Access. Vascular Access for Hemodialysis IX Symposium; May 6-7, 2004; Lake Buena Vista, FL. Page 74.

Davidson IJ, Brava K, Munschauer C, Nichols D. Conversion of failed native vein fistulas to PTFE grafts yields 90% access function at one year. Abstract presented at the 9th Biennial Symposium on Dialysis Access. Vascular Access for Hemodialysis IX Symposium; May 6-7, 2004; Lake Buena Vista, FL. Page 75.

Rooijens PPGM, Burgmans JJP, Tordoir JHM, et al. Autogenous radial-cephalic or prosthetic brachial-antecubital forearm loop AVF - A randomized prospective multicenter study of the patency of primary hemodialysis vascular access. Abstract presented at the 9th Biennial Symposium on Dialysis Access. Vascular Access for Hemodialysis IX Symposium; May 6-7, 2004; Lake Buena Vista, FL. Page 33.

Gallkowski U, Treiber W, Sures T. Preliminary results of a heparin bonded ePTFE graft for AV-access surgery. Abstract presented at the 9th Biennial Symposium on Dialysis Access. Vascular Access for Hemodialysis IX Symposium; May 6-7, 2004; Lake Buena Vista, FL. Page 96.

Davidson IJA, Munschauer CE. Preliminary experience with a new intrawall radially supported expanded PTFE graft. In: Henry ML, ed. *Vascular Access for Hemodialysis -VIII*. Arlington Heights, IL: W.L. Gore & Associates, Inc. & Access Medical Press; 2002:7:95-101.

Davidson IJA, Nichols D, Munschauer CE. PTFE graft survival following conversion from failed wrist native arteriovenous fistula. In: Henry ML, ed. *Vascular Access for Hemodialysis -VIII*. Arlington Heights, IL: W.L. Gore & Associates, Inc. & Access Medical Press; 2002:8:103-106.

Davidson IJA. PTFE bridge grafts. In: Davidson IJA, ed. *Access for Dialysis: Surgical & Radiologic Procedures*. 2nd Ed. Georgetown, TX: Landes Bioscience; 2002:4:45-81.

Bünger CM, Kröger J, Kock L, Henning A, Klar E, Schareck W. Axillary-axillary interarterial chest loop conduit as an alternative for chronic hemodialysis access. *Journal of Vascular Surgery* 2005;42(2):290-295.

- Davidson I, Munschauer C. Preliminary experience with a new intrawall radially supported ePTFE graft. Abstract presented at the 8th Biannual Symposium on Dialysis Access. Vascular Access for Hemodialysis VIII; May 9-10, 2002; Rancho Mirage, CA. Page 23.
- Benedetto B, Lipkowitz G, Madden R, *et al.* Use of cryopreserved cadaveric vein allograft for hemodialysis access precludes kidney transplantation because of allosensitization. *Journal of Vascular Surgery* 2001;34(1):139-142.
- Lumsden AB. Prospective, randomized multicenter trial of stepped Venaflo e-polytetrafluoroethylene grafts compared with Impra® stepped e-polytetrafluoroethylene grafts in hemodialysis. Abstract presented at the 7th Biannual Symposium in Dialysis Access. Vascular Access for Hemodialysis VII; May 4-5, 2000; San Antonio, TX. Page 11.
- Gagne PJ, Martinez J, DeMassi R, *et al.* The effect of a venous anastomosis Tyrell vein collar on the primary patency of arteriovenous grafts in patients undergoing hemodialysis. *Journal of Vascular Surgery* 2000;32(6):1149-1154.
- Hakaim AG, Scott TE. Durability of early prosthetic dialysis graft cannulation: results of a prospective, nonrandomized clinical trial. *Journal of Vascular Surgery* 1997;25(6):1002-1006.
- Veldenz HC, Lenz BJ, Dennis JW, Khansarinia S, Atteberry LR. Superiority of standard-thickness PTFE grafts in hemodialysis access. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-V*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1997:316-322.
- Hudson PC. Early cannulation of vascular access sites for dialysis. *Dialysis & Transplantation* 1996;25(8):523-526.
- Bartlett ST, Schweitzer EJ, Roberts JE, *et al.* Early experience with a new ePTFE vascular prosthesis for hemodialysis. *American Journal of Surgery* 1995;170(2):118-122.
- Brouwer DJ. Cannulation camp: basic needle cannulation training for dialysis staff. *Dialysis & Transplantation* 1995;24(11):606-612.
- Brouwer DJ. Hemodialysis: a nursing perspective. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-IV*. Chicago, IL: W.L. Gore & Associates, Inc. and Precept Press; 1995:131-151.
- Colonna JO II, Swanson J, Shaver TR. Successful early use of the stretch PTFE graft. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-IV*. Chicago, IL: W.L. Gore & Associates, Inc. and Precept Press; 1995:273-276.
- Dawidson IJA, ArRajab A, Melone LD, Poole T, Griffen D, Risser R. Early use of the GORE-TEX stretch graft. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-IV*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1995:109-117.
- Derenoncourt FJ. PTFE for A-V access: six years of experience with 310 reinforced and stretch grafts. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-IV*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1995:286-291.
- Tordoir JHM, Hofstra L, Leunissen KML, Kitslaar PJEHM. Early experience with stretch polytetrafluoroethylene grafts for haemodialysis access surgery: results of a prospective randomised study. *European Journal of Vascular & Endovascular Surgery* 1995;9(3):305-309.
- Tordoir JHM, Hofstra L, Bergmans DCJJ, Hoeks APG, Leunissen KML, Kitslaar JEHM. Stretch versus standard expanded PTFE grafts for hemodialysis access. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-IV*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1995:277-285.
- Sands JJ, Miranda CL. Prolongation of hemodialysis access survival with elective revision. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-IV*. Chicago, IL: W.L. Gore & Associates, Inc. and Precept Press; 1995:197-202.
- Hartigan MF. Vascular access and nephrology nursing practice: existing views and rationales for change. *Advances in Renal Replacement Therapy* 1994;1(2):155-162.
- Davidson I, Melone D. Preliminary experience with a new PTFE graft for vascular access. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-III*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1993:133-136.
- Simoni EJ, Jain KM, Munn JS. Use of 6 mm stretch PTFE grafts for early use in hemodialysis. In: Henry ML, Ferguson RM, eds. *Vascular Access for Hemodialysis-III*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1993:142-145.
- Taylor B, Sigley RD, May KJ. Fate of infected and eroded hemodialysis grafts and autogenous fistulas. *American Journal of Surgery* 1993;165(5):632-636.
- Mukherjee D. Rescue of failed forearm arteriovenous access grafts using an externally supported polytetrafluoroethylene graft. *American Journal of Surgery* 1993;166(3):306-307.
- Mayer DA, Zingale RG, Tsapogas MJ. Duplex scanning of expanded polytetrafluoroethylene dialysis shunts: impact on patient management and graft survival. *Vascular Surgery* 1993;27(9):647-658.
- Ballard JL, Bunt TJ, Malone JM. Major complications of angioaccess surgery. *American Journal of Surgery* 1992;164(3):229-232.
- Halstuk K, Berns A. Aneurysmal disease and puncture site complications in vascular access. In: Sommer BG, Henry ML, eds. *Vascular Access for Hemodialysis-II*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1991:75-84.
- Mehta S. Statistical summary of clinical results of vascular access procedures for hemodialysis. In: Sommer BG, Henry ML, eds. *Vascular Access for Hemodialysis-II*. Chicago, IL: W.L. Gore & Associates, Inc. & Precept Press; 1991:145-157.
- Pontari MA, McMillen MA. The straight radial-antecubital PTFE angio-access graft in an era of high-flux dialysis. *American Journal of Surgery* 1991;161(4):450-453.
- Schulak JA, Lukens ML, Mayes JT. Salvage of thrombosed forearm polytetrafluoroethylene vascular access grafts by reversal of flow direction and venous bypass grafting. *American Journal of Surgery* 1991;161(4):485-487.
- Hill SL, Donato AT. Complications of dialysis access: a six year study. *American Journal of Surgery* 1991;162(3):265-267.
- Fillinger MF, Reinitz ER, Schwartz RA, *et al.* Graft geometry and venous intimal-medial hyperplasia in arteriovenous loop grafts. *Journal of Vascular Surgery* 1990;11(4):556-566.
- Joffe B, Mordechay I. Conservative treatment of polytetrafluoroethylene graft infection. *Vascular Surgery* 1989;23(6):464-469.
- Rizzuti RP, Hale JC, Burkart TE. Extended patency of expanded polytetrafluoroethylene grafts for vascular access using optimal configuration and revisions. *Surgery, Gynecology & Obstetrics* 1988;166(1):23-27.
- Bell DD, Rosental JJ. Arteriovenous graft life in chronic hemodialysis: a need for prolongation. *Archives of Surgery* 1988;123(9):1169-1172.
- Zibari GB, Rohr MS, Landreneau MD, *et al.* Complications from permanent hemodialysis vascular access. *Surgery* 1988;104(4):681-686.
- McKenna PJ, Leadbetter MG. Salvage of chronically exposed Gore-Tex vascular access grafts in the hemodialysis patient. *Plastic & Reconstructive Surgery* 1988;82(6):1046-1049.
- Raju S. PTFE grafts for hemodialysis access: techniques for insertion and management of complications. *Annals of Surgery* 1987;206(5):666-673.
- Rittgers SE, Garcia-Valdez C, McCormick JT, Posner MP. Noninvasive blood flow measurement in expanded polytetrafluoroethylene grafts for hemodialysis access. *Journal of Vascular Surgery* 1986;3(4):635-642.
- Fivush BA, Bock GH, Guzzetta PC, Salcedo JR, Ruley EJ. Vancomycin prevents polytetrafluoroethylene graft infections in pediatric patients receiving chronic hemodialysis. *American Journal of Kidney Diseases* 1985;5(2):120-123.
- Tanchajja S, Mohaideen AH, Avram MM, Eisenberg MM. Management of infection associated with prosthetic graft exposure in angioaccess. *Vascular Surgery* 1985;19(2):117-121.
- Mandel SR, McDougal EG. Popliteal artery to saphenous vein vascular access for hemodialysis. *Surgery, Gynecology & Obstetrics* 1985;160(4):358-359.
- Moosa HH, Peitzman AB, Thompson BR, Webster MW, Steed DL. Salvage of exposed arteriovenous hemodialysis fistulas. *Journal of Vascular Surgery* 1985;2(4):610-612.
- Taucher LA. Immediate safe hemodialysis into arteriovenous fistulas created with a new tunnel: an 11 year experience. *American Journal of Surgery* 1985;150(2):212-215.
- Hinsdale JG, Lipkowitz GS, Hoover EL. Vascular access for hemodialysis in the elderly: results and perspectives in a geriatric population. *Dialysis & Transplantation* 1985;14(10):560-565.
- Gifford RRM. Management of tunnel infections of dialysis polytetrafluoroethylene grafts. *Journal of Vascular Surgery* 1985;2(6):854-858.
- Majeski JA. Forearm arterial venous shunt for hemodialysis. *American Surgeon* 1985;51(11):630-631.
- Collier PE, Saracco GM, Diamond DL. Streptokinase and transluminal angioplasty in reclamation of AV fistula. *Contemporary Surgery* 1984;24:69-71.
- Connolly JE, Brownell DA, Levine EF, McCart PM. Complications of renal dialysis access procedures. *Archives of Surgery* 1984;119(11):1325-1328.
- Anderson CB, Sicard GA, Etheredge EE. Primary and secondary operations for vascular access. In: Bergan JJ, ed. *Evaluation and Treatment of Upper and Lower Extremity Circulatory Disorders*, Pennsylvania, PA: Grune & Stratton; 1983:279-306.
- Etheredge EE, Haid SD, Maeser MN, Sicard GA, Anderson CB. Salvage operations for malfunctioning polytetrafluoroethylene hemodialysis access grafts. *Surgery* 1983;94(3):464-470.
- Slooff MJH, Smits PJH, Lichtendahl DHE, Van Der Hem GK. Non-thrombotic complications of PTFE grafts for hemodialysis. *Proceedings of the European Dialysis & Transplant Association* 1982;19:234-237.
- Hodgkinson DJ, Shepard GH. Coverage of exposed GORE-TEX dialysis access graft with local sublimis myocutaneous flap. *Plastic & Reconstructive Surgery* 1982;69(6):1010-1012.
- Sabanayagam P, Sorkin HL, Soricelli RR, Clark JE. A prospective random study comparing GORE-TEX graft and bovine graft A.V. fistulae for maintenance hemodialysis. *Journal of the European Society for Artificial Organs* 1982:8-14.
- Bolton W, Cannon JA. Seroma formation associated with PTFE vascular grafts used as arteriovenous fistulae. *Dialysis & Transplantation* 1981;10(1):60-63.
- Humphries Jr. AL, Nesbit Jr. RR, Caruana RJ, Hutchins RS, Heimbarger RA, Wray CH. Thirty-six recommendations for vascular access operations: lessons learned from our first thousand operations. *American Surgeon* 1981;47(4):145-151.
- Rapaport A, Noon GP, McCollum CH. Polytetrafluoroethylene (PTFE) grafts for haemodialysis in chronic renal failure: assessment of durability and function at three years. *Australian & New Zealand Journal of Surgery* 1981;51(6):562-567.
- Anderson CB, Etheredge EE, Sicard GA. One hundred polytetrafluoroethylene vascular access grafts. *Dialysis & Transplantation* 1980;9(3):237-238.
- Anderson CB, Etheredge EE. Subcutaneous tunnel for vascular access grafts for hemodialysis. *Surgery, Gynecology & Obstetrics* 1980;150(4):569-570.
- Rosental JJ, Bell DD, Gaspar MR, Movius HJ, Lemire GG. Prevention of high flow problems of arteriovenous grafts. *American Journal of Surgery* 1980;140(2):231-233.
- Anderson CB, Sicard GA, Etheredge EE. Bovine carotid artery and expanded polytetrafluoroethylene grafts for hemodialysis vascular access. *Journal of Surgical Research* 1980;29(2):184-188.
- Sabanayagam P, Schwartz AB, Soricelli RR, Lyons P, Chinitz J. A comparative study of 402 bovine heterografts and 225 reinforced expanded PTFE grafts as AVF in the ESRD patient. *Transactions - American Society for Artificial Internal Organs* 1980;1(26):88-91.



W. L. Gore & Associates, Inc.

Flagstaff, AZ 86004

美国戈尔公司

电话: +86.21.51728299 (大中华地区)

电话: 00800.6334.4673 (欧洲)

电话: 1.800.437.8181 (美国)

电话: 928.779.2771 (美国)

goremedical.com

所列产品并非在所有的市场有售。

GORE®、GORE-TEX®、ACUSEAL、PERFORMANCE THROUGH INNOVATION及其设计为W. L. Gore & Associates的商标。
© 2012 W. L. Gore & Associates, Inc. 版权所有。 AP0064-CH1 2012年1月